

1 2 3 4 5 6 7 8


REV	ECN	DESCRIPTION	DESIGN	CHECK	CHECK/R&D	APPR DATE
D	EAF074	增加IPX7和P/N 调整版式等	杨义鹏	傅小波	汪新兵 王彦	07. 2.16
E		增加警告标志和调整版式等				

A


B

C

D

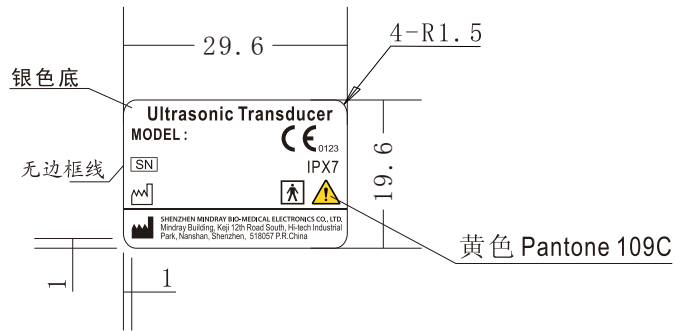

出纸方向

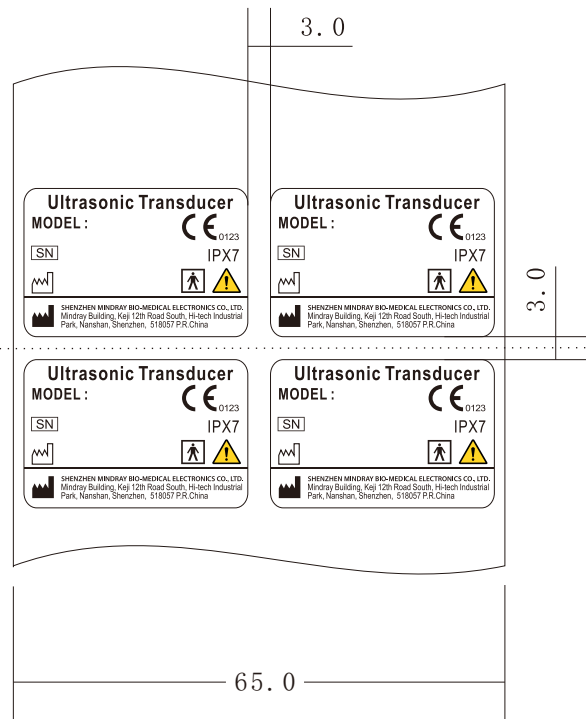

技术要求

- 1、文字与图形的大小及位置等以电子文档1: 1为准
未注印刷颜色为黑色;
- 2、按图示卷成一卷,裁切时不得切伤感光底纸;
- 3、图上未注公差±0.3mm;
- 4、来料时在卷筒内径上贴物料标贴: PR2A-20-17302E;
- 5、底材要求用格拉辛半透明感光底纸。

File	Bytes
Date	Time
Software & Rev: CorelDraw 12.0	

机密: 此图及其全部知识产权(含著作权)归深圳迈瑞生物医疗电子股份有限公司所有。未经深圳迈瑞生物医疗电子股份有限公司预先书面许可, 严禁出于任何目的, 对此图的全部或部分内容(包括但不限于图中信息、数据、运算结果等)使用、拷贝或复制。
CONFIDENTIAL DISCLOSURE: This set of drawing(s) and all its intellectual property right s(including copyright) subsisting herein are property of Shenzhen Mindray Bio-medical Electronics Co., Ltd. No use, copies or reproductions should be made of this drawing or any part(s) thereof for whatever purpose nor shall any information, data, calculations, or other contents contained in this drawing be disseminated without prior written permission of Shenzhen Mindray Bio-medical Electronics Co., Ltd.

APPROVALS		DATE	MINDRAY		
DESIGN	吴言	02.12.25	TITLE 探头插座标贴(左侧)		
CHECK	曾云泉	02.12.25			
CHECK	郭根苗	03.02.19	DWG NO.	C-PR2A-20-17302	
CHECK	/	/	MATERIAL	亚银PET72826	REV. E
R&D	杨旭	02.12.25	SCALE 1/1	ATTR. 其它	SIZE A4
CHIEF ENG.	郭宏凌	02.12.26	PROJECTION	⊕ ⊖	SHEET 1 OF 1